

+
1/2

FIG.1

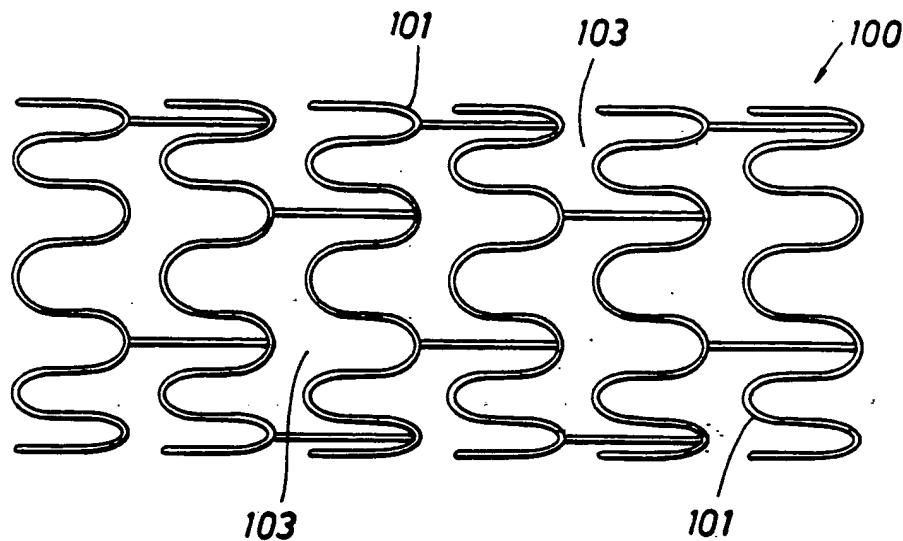
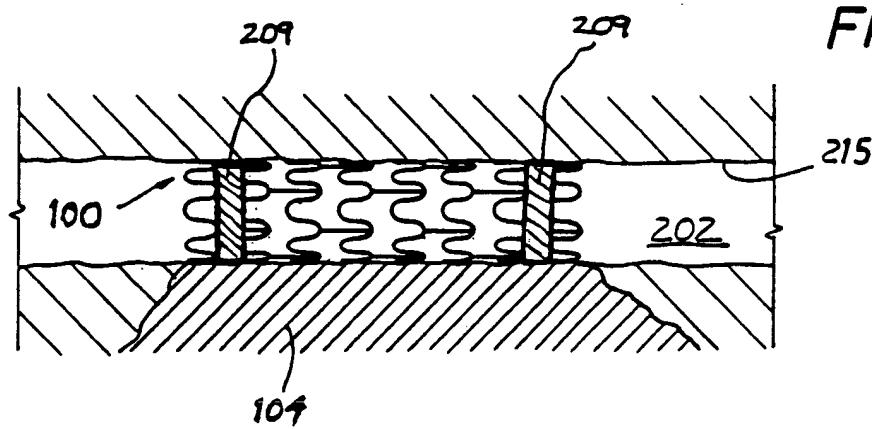


FIG.2



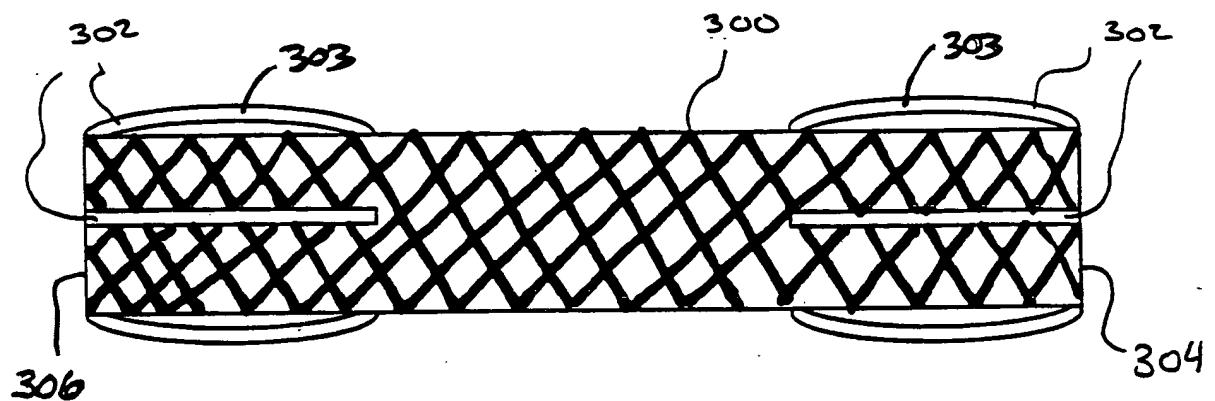


FIG. 3

PREPARE VISCOUS SOLUTION AND PLACE IN
CONTAINER HAVING A DRIP NOZZLE

~401

ROTATABLY POSITION STENT NEAR DRIP NOZZLE

~402

DRIP VISCOUS SOLUTION ONTO ROTATING STENT

~403

STOP FLOW OF VISCOUS SOLUTION AND CURE
BAND IN SITU

~404

REPEAT OPERATIONS 401 - 404 IF DESIRED

~405

STERILIZE STENT AND BAND

~406

PACKAGE STENT IN STERILE CONTAINER

~407

FIG. 4

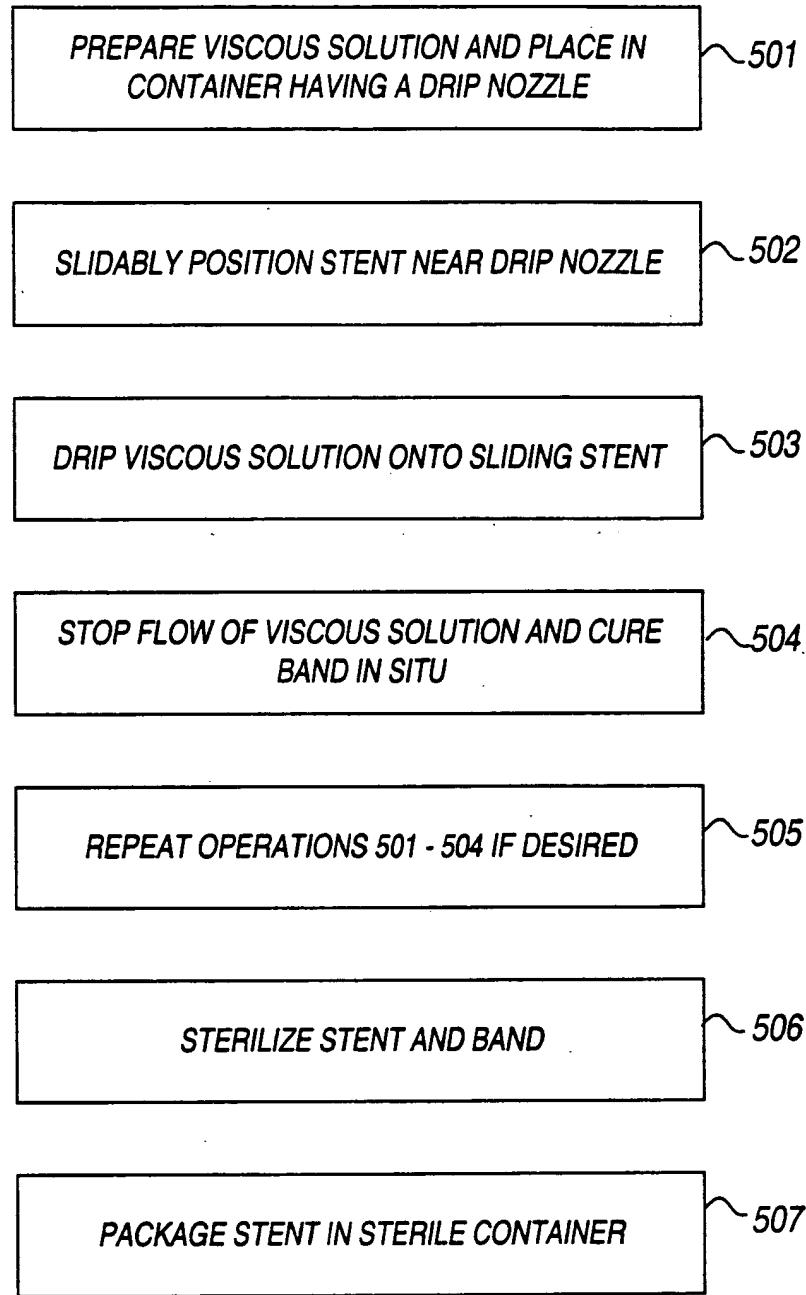


FIG. 5

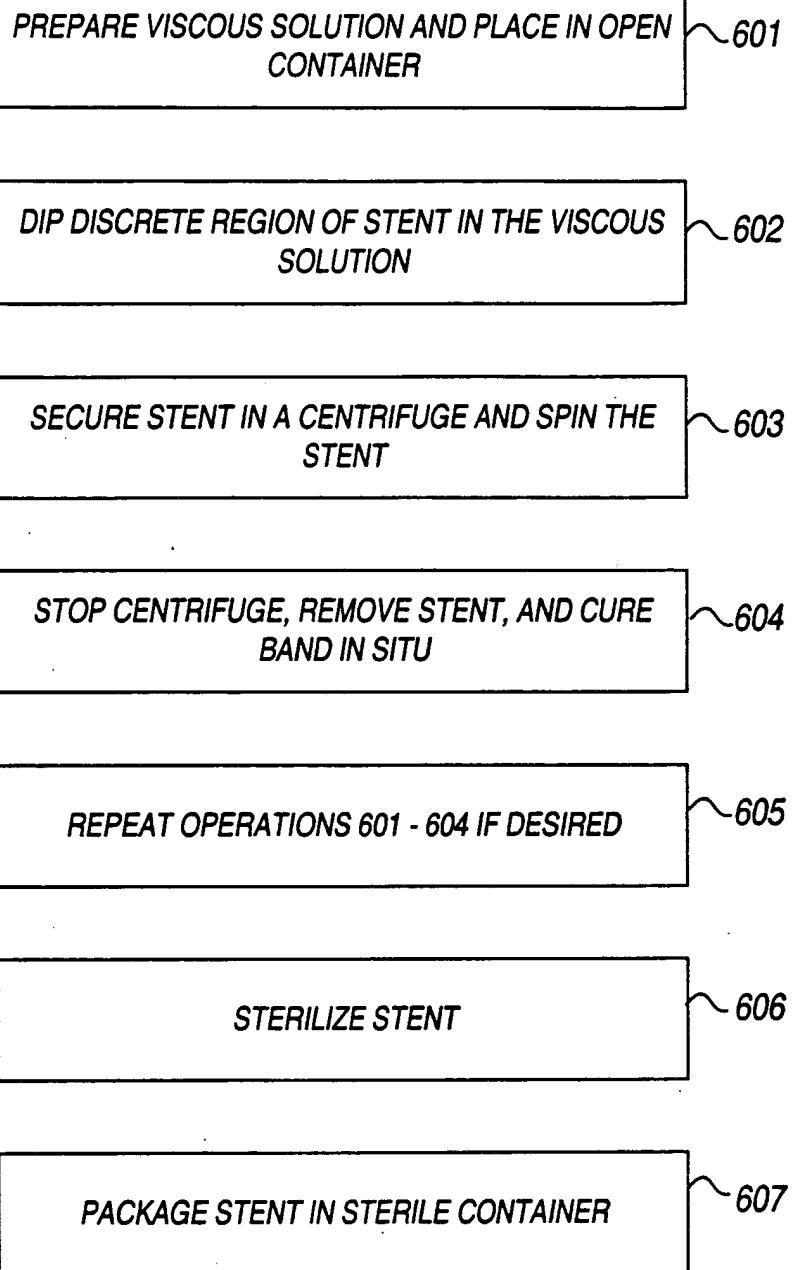


FIG. 6